
ICS 17.220.00; 29.020

Descriptors: Electromagnetic compatibility, measurements, tests, anechoic chambers, specifications

English version

Anechoic chambers

Part 1: Shield attenuation measurement

Chambres anéchoïques
Partie 1: Mesure d'atténuation de blindage

Absorberräume
Teil 1: Schirmdämpfungsmessung

This European Standard was approved by CENELEC on 1995-07-04. CENELEC members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CENELEC member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CENELEC members are the national standards bodies of Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

CENELEC

European Committee for Electrotechnical Standardization
Comité Européen de Normalisation Electrotechnique
Europäisches Komitee für Elektrotechnische Normung

Central Secretariat: rue de Stassart 35, B-1050 Brussels

Foreword

This European Standard was prepared by working group WG 4 of CENELEC Technical Committee TC 210, EMC.

It was submitted to the CENELEC Unique Acceptance Procedure (UAP) in August 1994 and was approved by CENELEC as EN 50147-1 on 1995-07-04.

The following dates were fixed:

- latest date by which the EN has to be implemented at national level by publication of an identical national standard or by endorsement (dop) 1996-09-01
- latest date by which national standards conflicting with the EN have to be withdrawn (dow) 1996-09-01

Contents

	Page
Foreword	2
1 Scope	3
2 Normative references	3
3 Definitions	3
4 General points relating to shielding effectiveness	3
4.1 Shielding	3
4.2 Shield attenuation	3
5 Shield attenuation measurement	5
5.1 Test equipment	5
5.2 Acceptance tests	5
5.3 Reference level	6

1 Scope

This standard applies to measurements of shielding attenuation of shielded enclosures (chambers, rooms) in the frequency range 9 kHz – 40 GHz. The object of this standard is to establish a common measurement procedure for validating the shielding effectiveness of a shielded enclosure.

2 Normative references

This European Standard incorporates by dated or undated reference, provisions from other publications. These normative references are cited at the appropriate places in the text and the publications listed hereafter. Dated references, subsequent amendments to or revisions of any of these publications apply to this European Standard only when incorporated in it by amendment or revision. For undated references the latest edition of the publication referred to applies.

IEC 50(161) 1990 *International Electrotechnical Vocabulary (IEV)*
Chapter 161: Electromagnetic Compatibility

3 Definitions

For the purposes of this standard the definitions contained in IEC 50(161) apply.

4 General points relating to shielding effectiveness

4.1 Shielding

Shield attenuation can be calculated only in ideal cases. The most significant factor is that the shielded enclosure should be homogeneous and consist of materials whose properties are defined in every respect. In practice, deviations from these conditions may be so great that the calculation results only in approximate values.

4.2 Shield attenuation

The shield attenuation is given by (see figure 1):

$$a_s = 20 \log(E_0/E_1) \text{ for the electric field}$$

$$a_s = 20 \log(H_0/H_1) \text{ for the magnetic field}$$

where:

a_s is the shield attenuation in dB.

E_0 and H_0 are the E and H field strengths at a location without shielding between the transmitting and receiving antennas (reference level).

E_1 and H_1 are the E and H field strengths at the same location as above with shielding between the transmitting and receiving antennas.

Figure 2 shows typical shield attenuation values of a state of the art shielded enclosure.


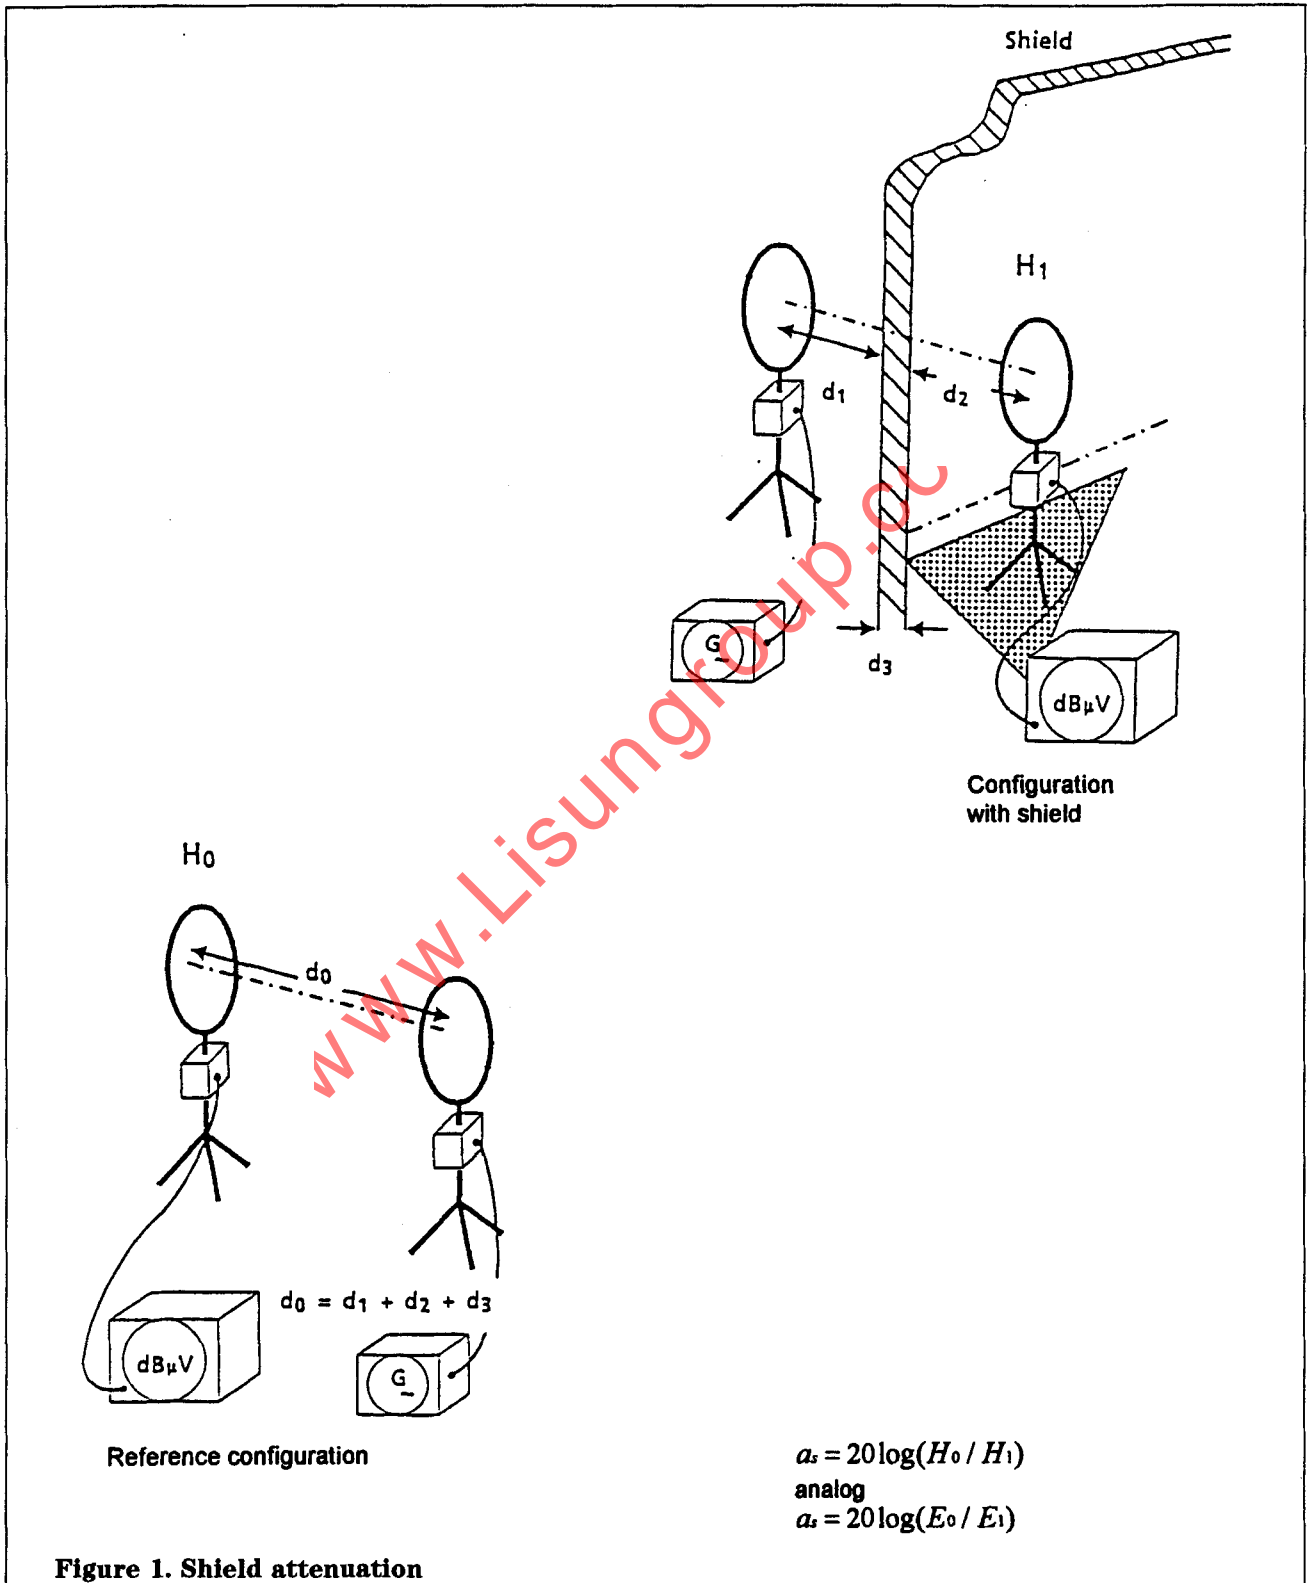


Figure 1. Shield attenuation

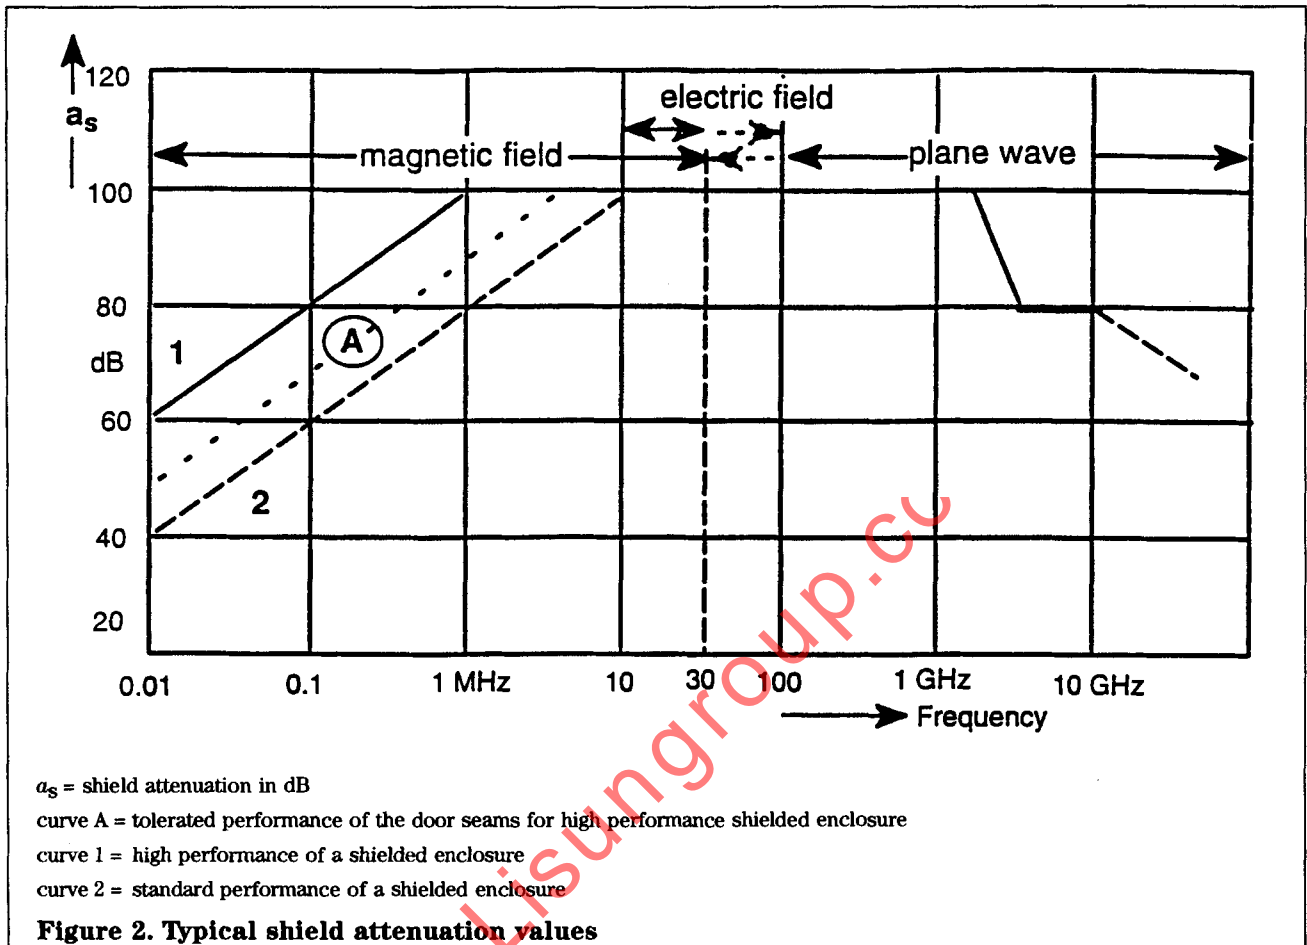

5 Shield attenuation measurement

The measurement is normally carried out with all the shielding components in place and, in the case of filters, with all wires and cables connected.

NOTE. The procedure is derived from NSA 65-6-October 1964; National Security Agency Specification for R.F. Shielded Enclosures for Communication Equipment.

5.1 Test equipment

The following types of equipment shall be used in performing the shield attenuation test, depending on the frequency range given in the specification of the enclosure. The measurement equipment shall have sufficient dynamic range to enable the test to be performed:

- CW signal sources covering 9 kHz to 40 GHz with adequate frequency stability. If unavailable in the microwave region (1 – 40 GHz), pulsed sources may be substituted;

NOTE. The starting frequency for shield attenuation measurements may be 10 kHz if the measurement equipment offers no other alternative.

- loop antennas for magnetic field measurements;
- tunable or broadband dipoles, monopoles with ground planes for electric field and plane wave measurements, and horn antennas for plane waves at microwave frequencies;
- probes for joint leakage tests;
- receivers with adequate sensitivity.

5.2 Acceptance tests

Acceptance tests shall be performed in accordance with the procedures described below and illustrated in figures 3 and 4.

Measurements shall be taken at several positions around the enclosure as given in the specification of the enclosure. In general, these measurements are made before absorber installation.


If the ambient noise level is low enough, all tests should be run with the receiver outside and the transmitter inside the enclosure.

5.2.1 Leakage test

Prior to acceptance tests leakage tests should be made all around the door frame, through accessible joints, around the filters and all around the air ducts. In addition, the magnitude and location of the maximum signal level emanating from the enclosure should be found by moving the antennas to at least four locations, preferably on different walls.

5.2.2 Electric and magnetic field measurements

Electric and magnetic field attenuation tests (reference measurements) shall be made with the antennas located directly opposite each other and separated by a distance shown in figures 3 and 4 plus the wall thickness.

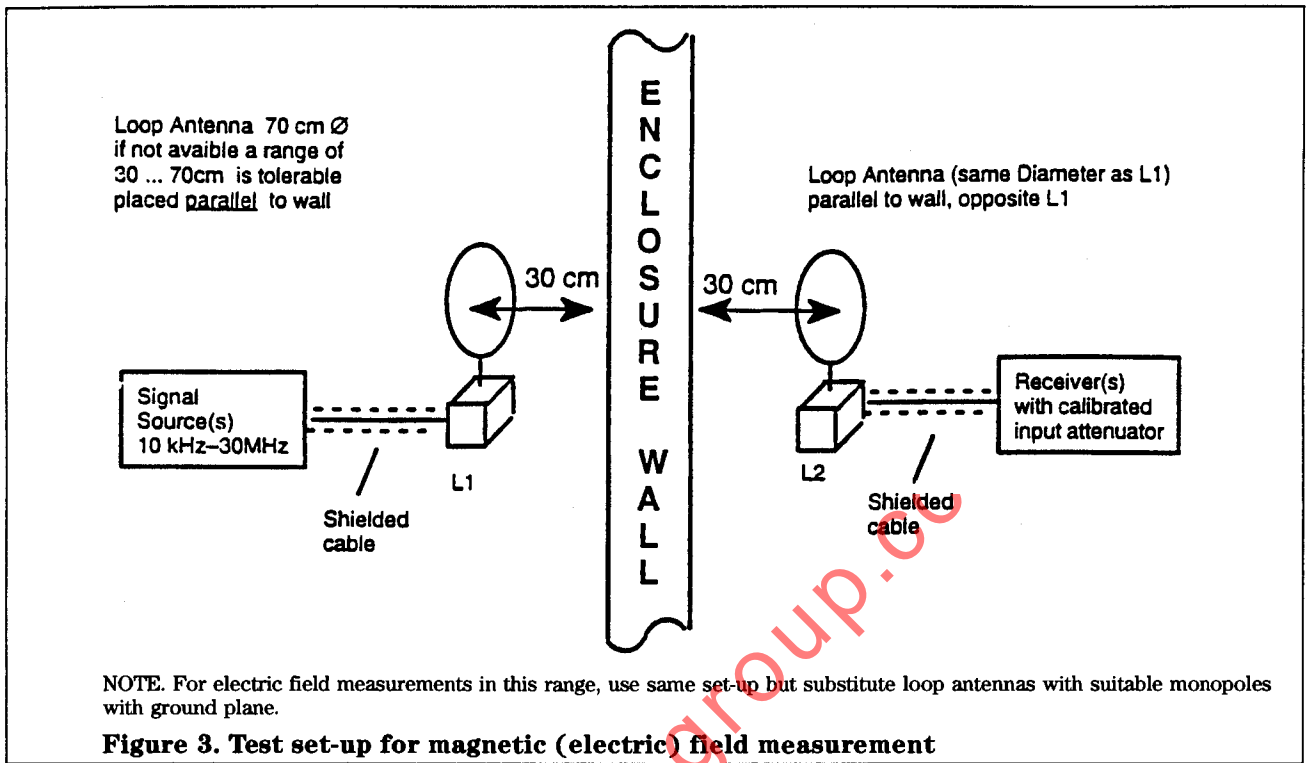

Magnetic fields shall be measured with the loops parallel to a wall panel directly opposite each other.

Recommended test frequencies for magnetic fields are 10 kHz, 100 kHz, 1MHz, 10 MHz and 30 MHz and 10 MHz and 30 MHz for electric field.

5.2.3 Plane wave measurements

Measurements shall be taken at the frequencies 100 MHz, 400 MHz, 1 GHz, 10 GHz and 40 GHz at least, depending on the frequency range given in the specification of the enclosure.


The test set-up is shown in figure 4.

5.3 Reference level

When undertaking the reference measurement it is important to note that in many countries the transmission of radio frequency energy is licensed and reference must be made to the country authority to determine if any such regulations apply. After the country requirements have been satisfied the reference measurement shall be made in the following manner.

The reference level shall be recorded with the outside antenna position unchanged and the inside antenna moved outside and positioned opposite plus a distance equivalent to the wall thickness. The value of signal levels may be recorded in decibels [dB] relative to 1 microvolt or 1 mW.

If local country provisions preclude the determination of the reference level as described above, alternative methods may be used provided these give technically equivalent results.

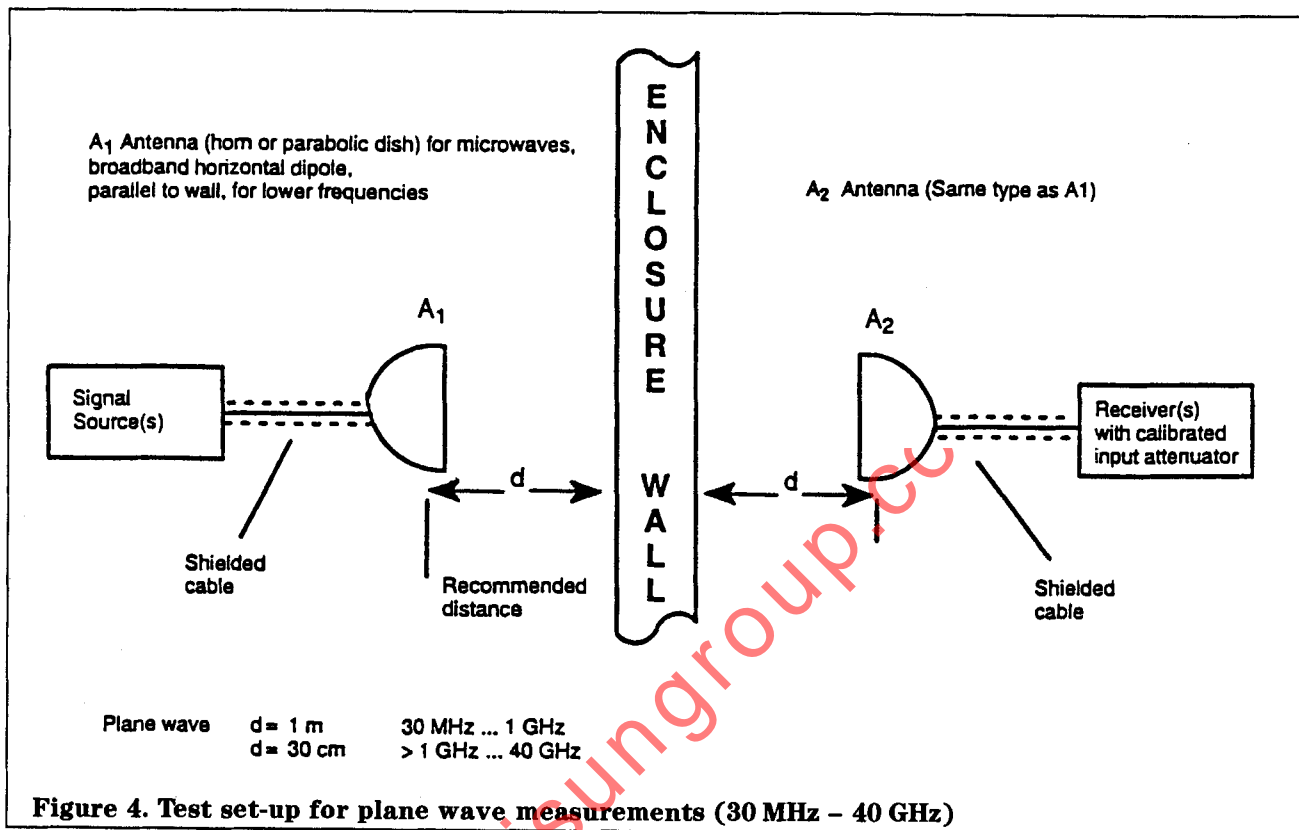

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Contract requirements

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the responsible technical committee, the identity of which can be found on the inside front cover. Tel: 0181 996 9000; Fax: 0181 996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services, Sales Department at Chiswick: Tel: 0181 996 7000; Fax: 0181 996 7001.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library, the Standardline Database, the BSI Information Technology Service (BITS) and its Technical Help to Exporters Service. Contact the Information Department at Chiswick: Tel: 0181 996 7111; Fax: 0181 996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Customer Services, Membership at Chiswick: Tel: 0181 996 7002; Fax: 0181 996 7001.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager, BSI, 389 Chiswick High Road, London W4 4AL.